


# Ultrasound advanced imaging: beyond anatomy!


Hervé Liebgott  
Associate Prof. University of Lyon  
CREATIS

# Introduction

Objective n° 1 in medical imaging: anatomy

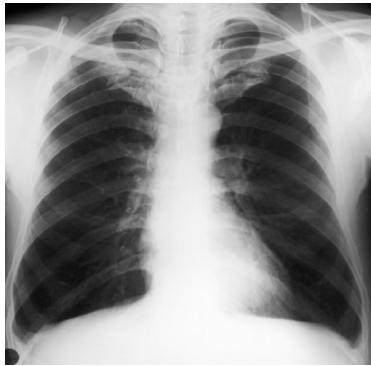

X-ray

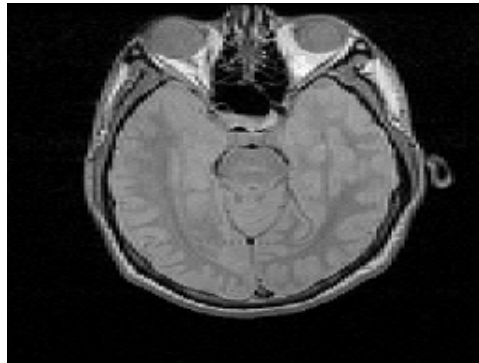

MRI



Ultrasound

What else?

Function – Tissue characterization

# Examples and the corresponding evolution of ultrasound imaging

Part 1

- static elastography
- shear wave elastography
- ultrafast imaging
- photo-acoustic imaging

# Tissue elasticity imaging - clinical motivation

- The objective of elastography is to produce a map of the stiffness of tissues
- There is strong correlation between stiffness and some pathologies

## Young Modulus in Breast tissue (kPa)

<b>Normal fat</b>	<b>: <math>18 \pm 7</math></b>
<b>Normal glandular</b>	<b>: <math>28 \pm 14</math></b>
<b>Infiltrating carcinoma</b>	<b>: <math>106 \pm 32</math></b>


## Young Modulus in Prostate tissue (kPa)

<b>Normal anterior</b>	<b>: <math>60 \pm 15</math></b>
<b>Normal posterior</b>	<b>: <math>68 \pm 14</math></b>
<b>Cancer</b>	<b>: <math>230 \pm 34</math></b>


[Krouskop-98]

- The principle of static elastography is to image the deformation of a tissue under external load (palpation with the US probe)


# Elastography - Basic principle

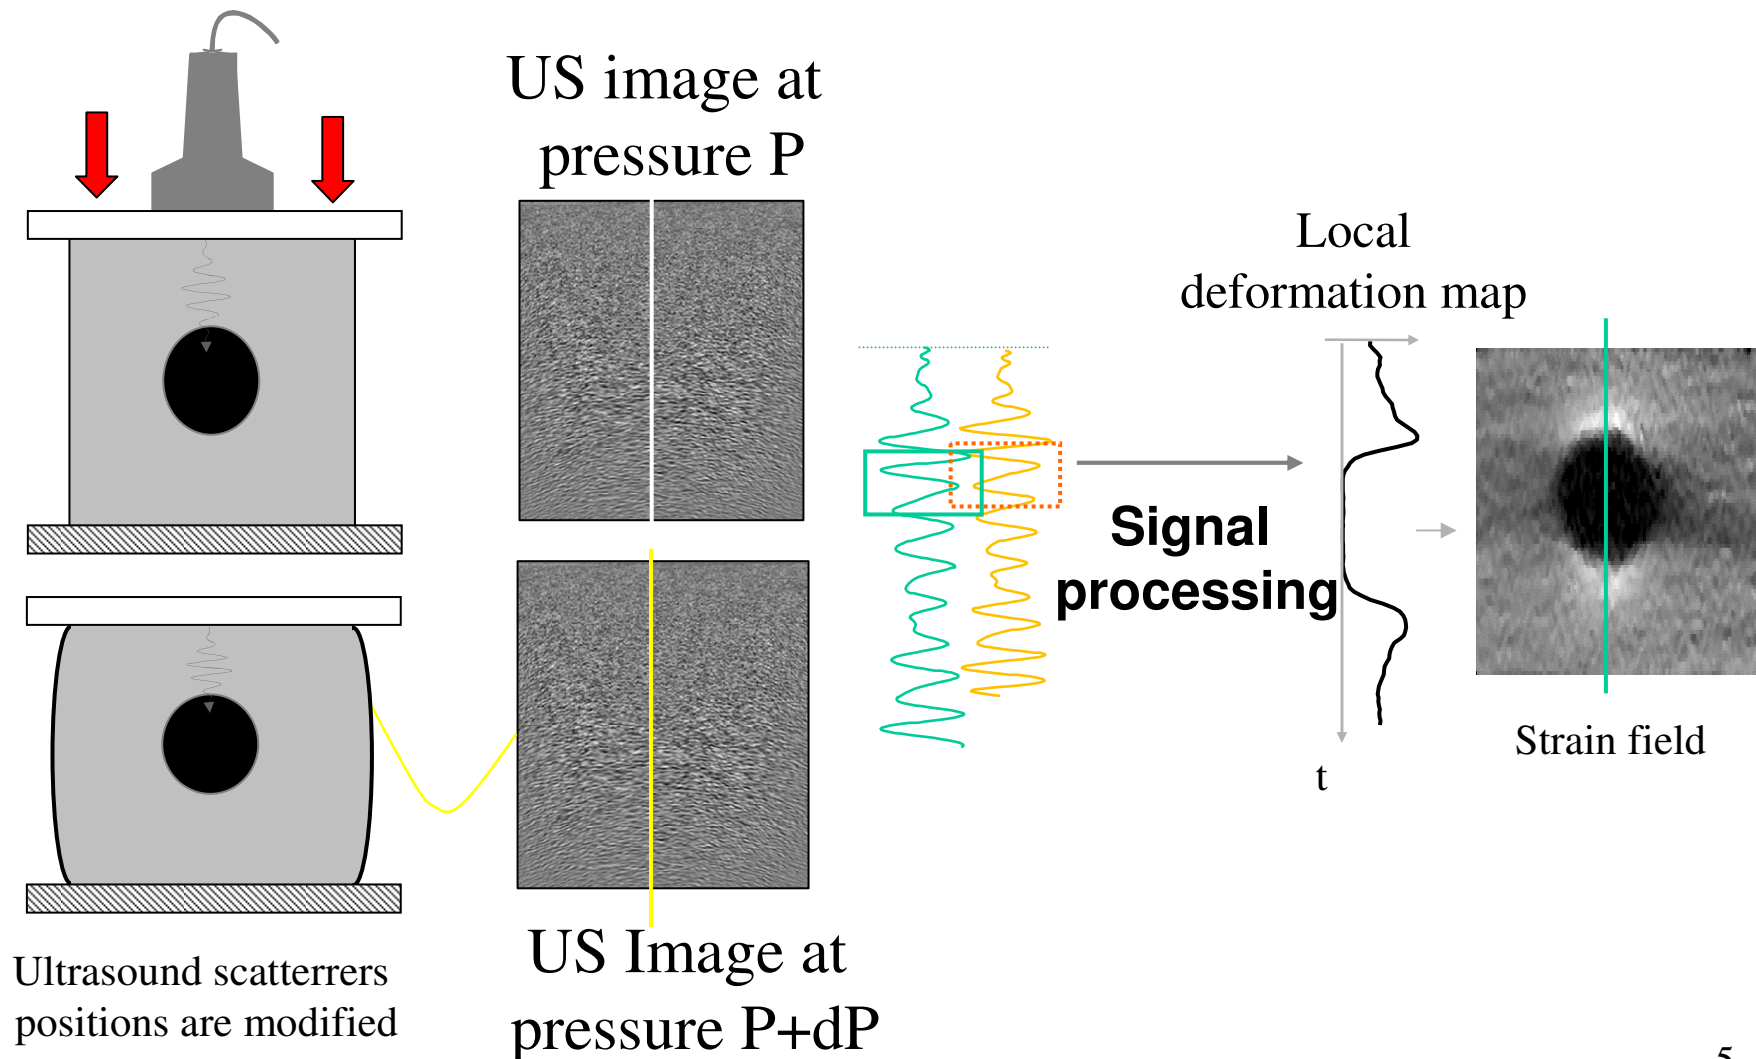

# *In vitro* results: experimental set-up

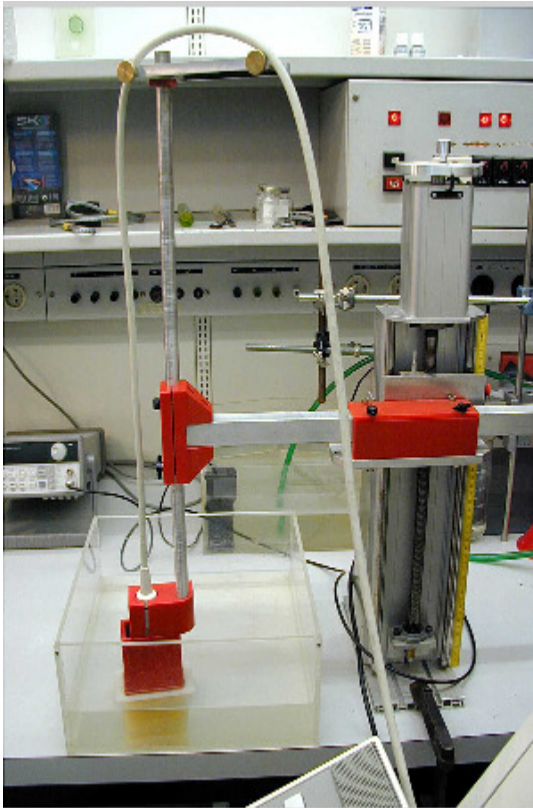

Bochum

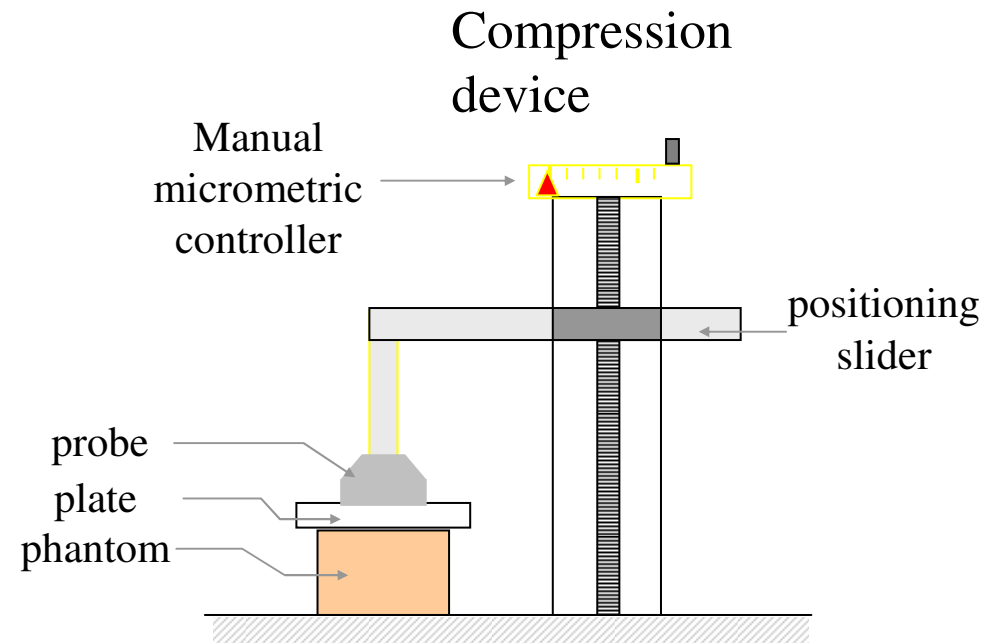


Central frequency: 7.2 MHz

Sampling frequency: 36 MHz


Displacement step precision: 0.05 mm

# Results with a foam phantom

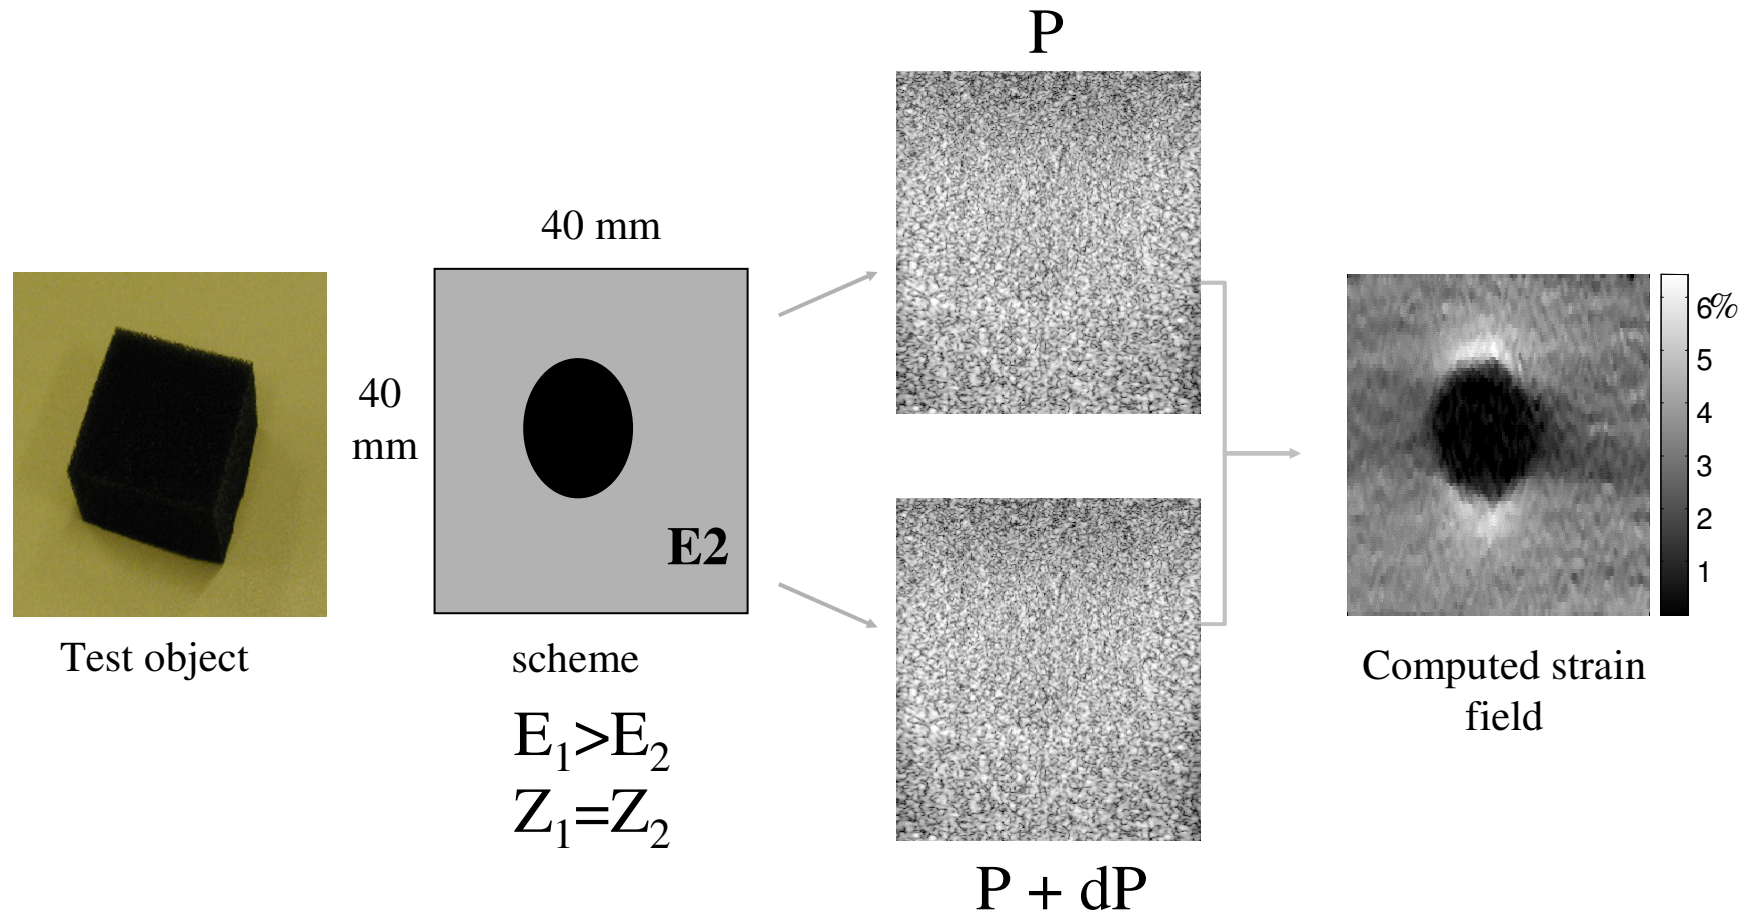

- Foam phantom containing a spherical hard inclusion in agar (diameter: 1.5 cm)
- phantom characteristics: acoustical homogeneity; compressibility
- elastogram computation: window length = 1 mm, 60 % overlap


# Results with a 3-layer tissue mimicking phantom

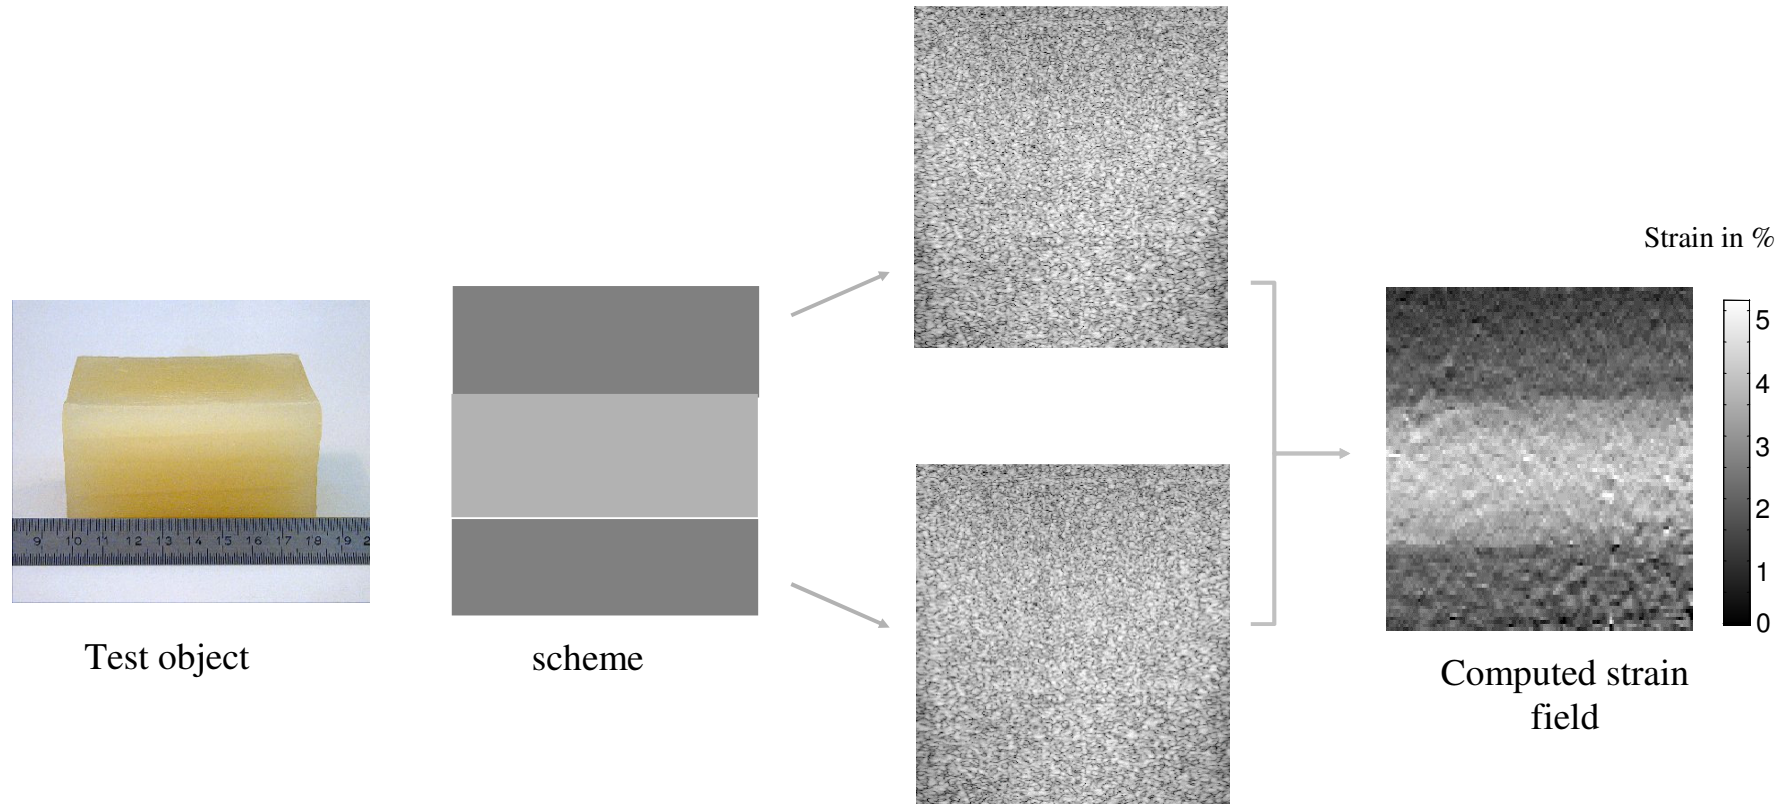


- 3-layer phantom
  - soft layer: 6% gelatine, 1% agar, 1% scatterers (SiC)
  - hard layer: 6% gelatine, 4.5% agar, 1% scatterers
- elastogram computation window length: 1 mm 60 % overlap




# Results with a two layer cryogel phantom

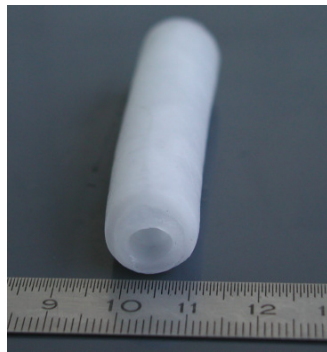


Photograph

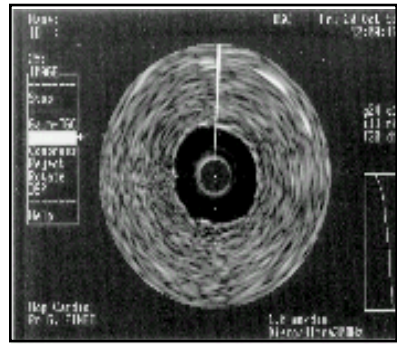


B mode image

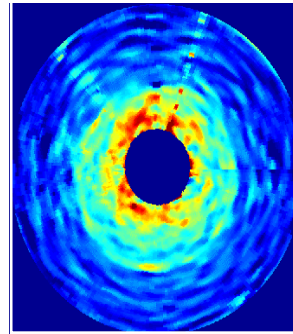

Elastogram

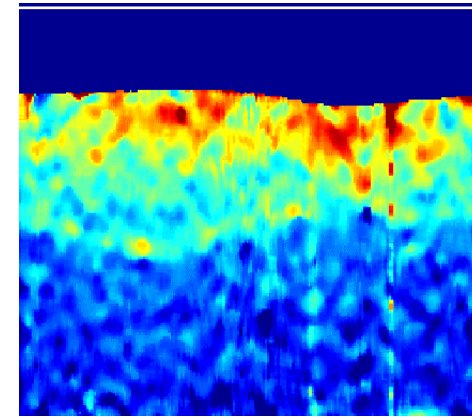


Strain in %



- Polyvinyl alcohol cryogel phantom
- 2 layers : soft = 1 freeze-thaw cycle, hard = 3 freeze-thaw cycle
- elastogram computation : window length = 0.25 mm, 80% overlap

# Results with a fresh excised carotid artery

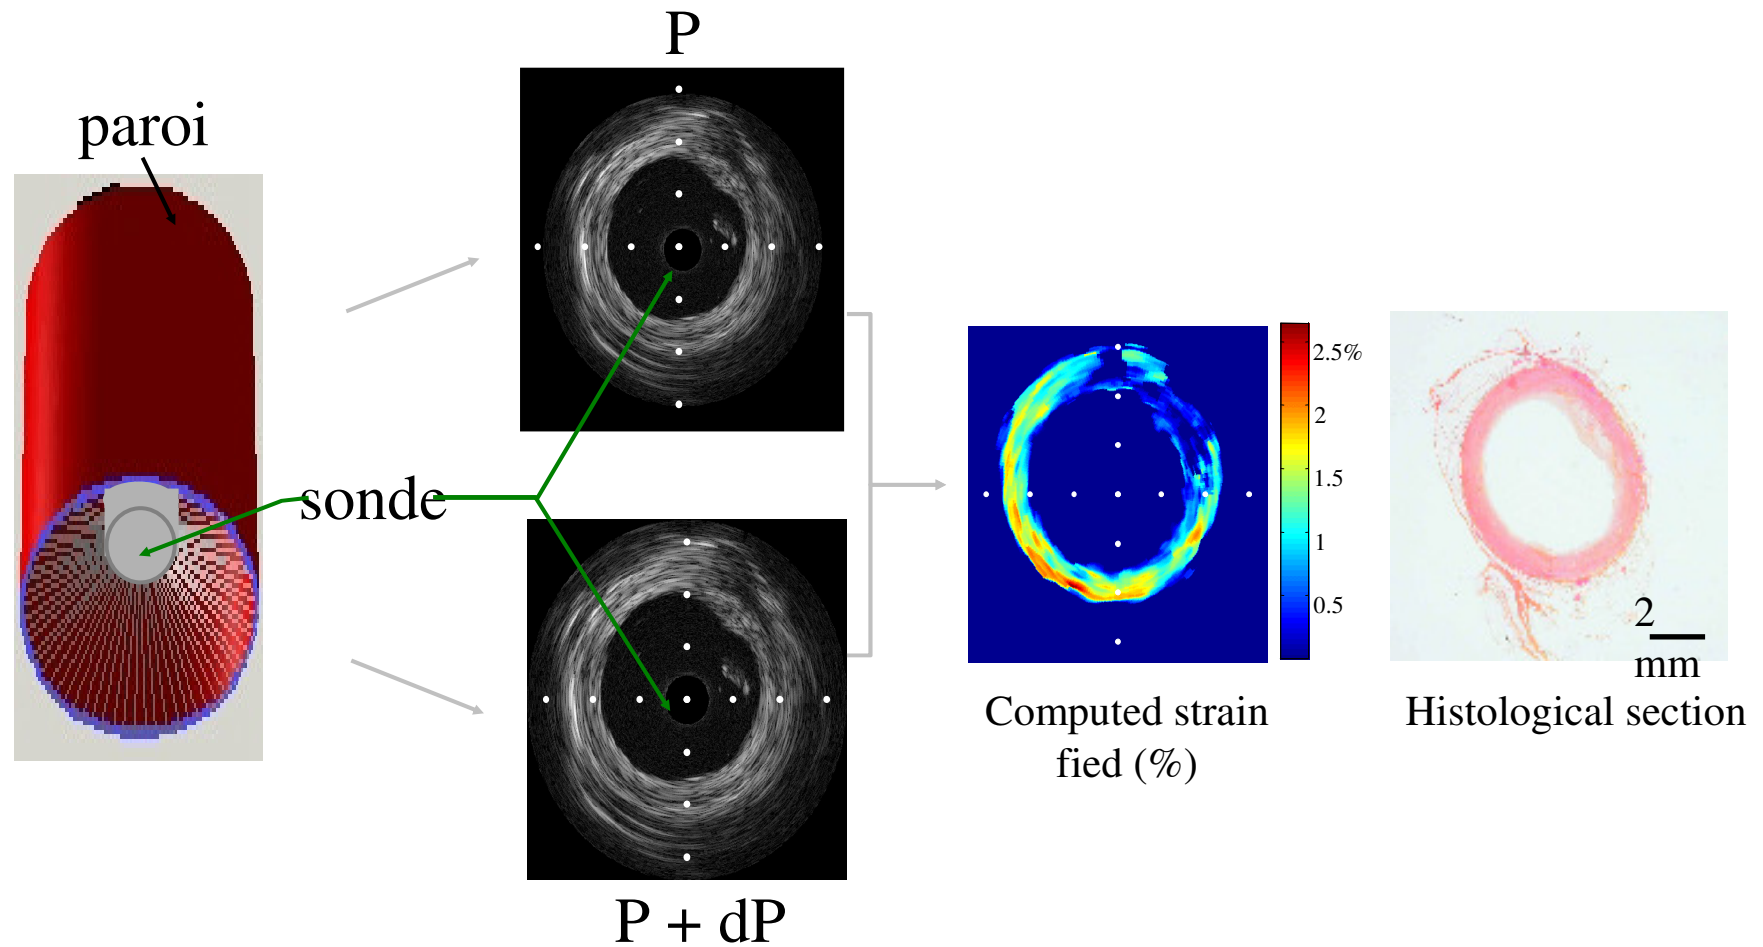

# Limitation of static elastography

Only qualitative / relative stiffness


Depends on the applied load

Not quantitative

➔ Shear wave elastography

# The idea of shear wave elastography

Shear wave propagation velocity is proportional to shear modulus

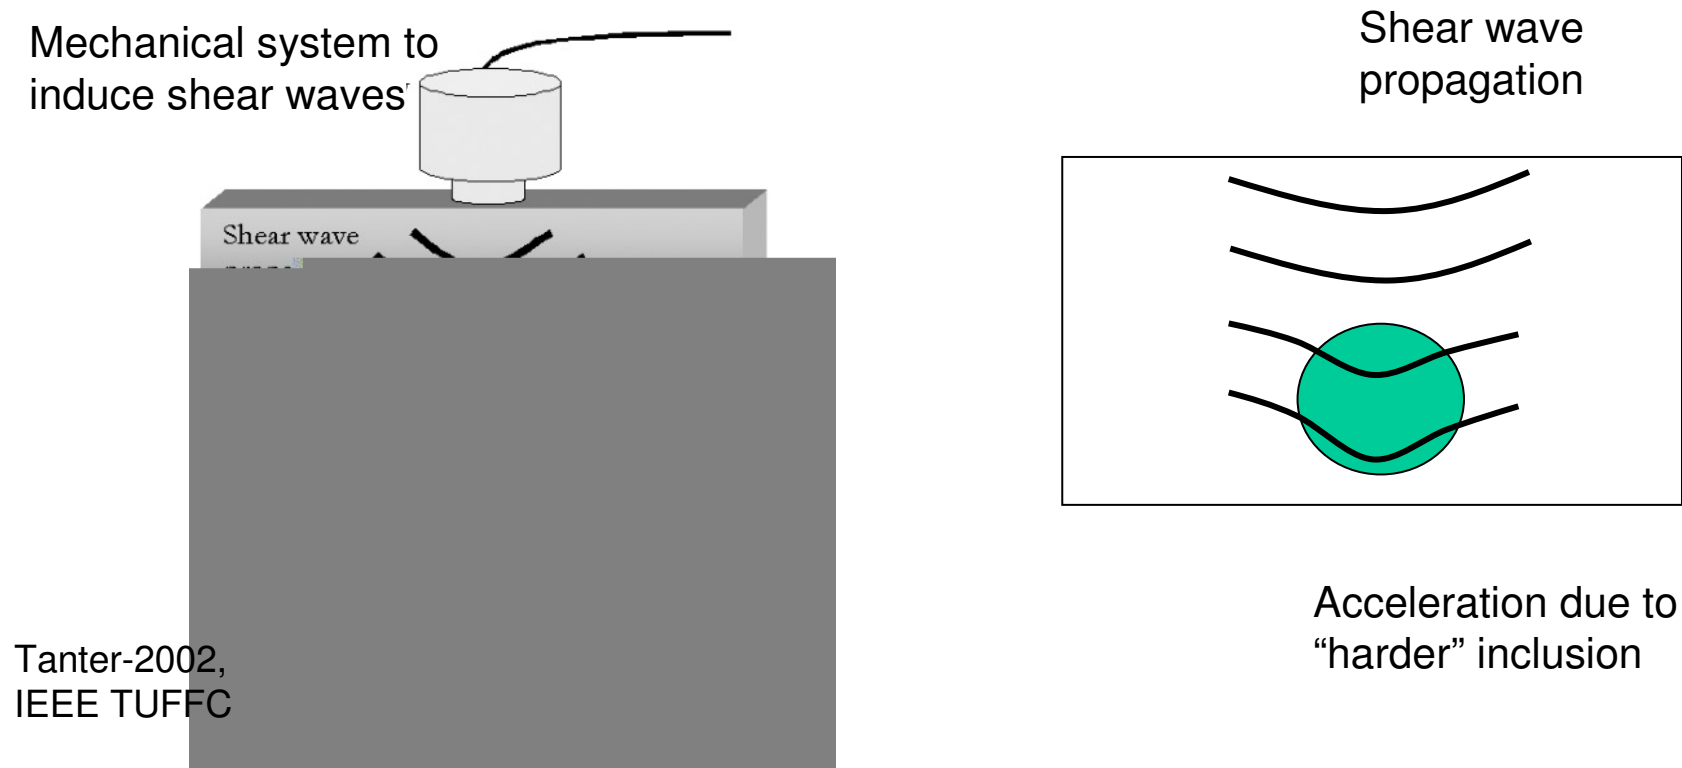

US Imaging of the shear wave propagation +  
determination of local velocity → shear wave modulus

# Shear wave elastography




Shear wave have typical velocities ranging between 1-10m.s<sup>-1</sup>

→ imaging at frame rate  $\gg 1$  KHz is needed

How can ultrafast imaging be performed??

Use **broad field-of-view transmit beams** with **full parallel receive beamforming**: 1 image per pulse => **4-5000 fps!**


### Focused pulses

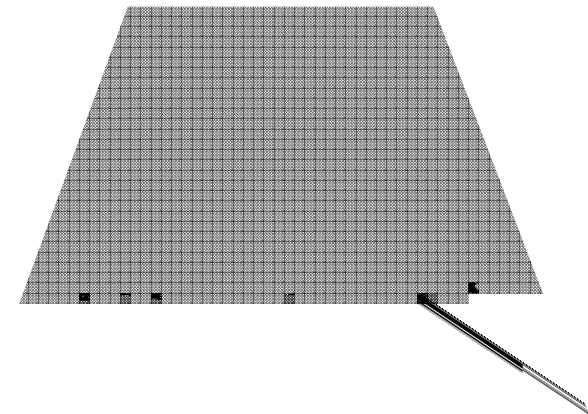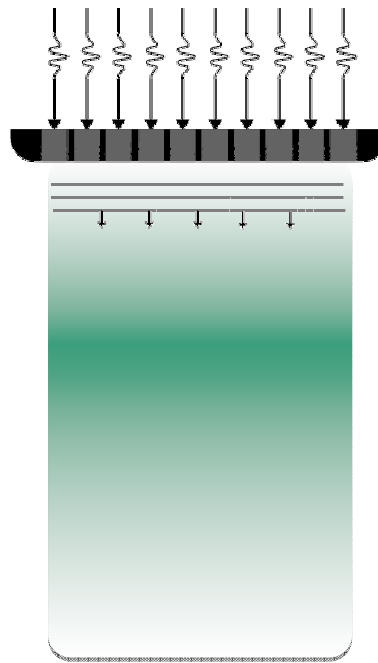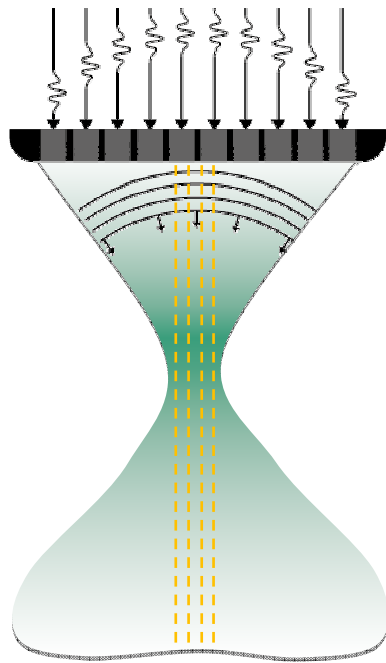

# Conventional vs ultrafast imaging



## Conventional ultrasound imaging

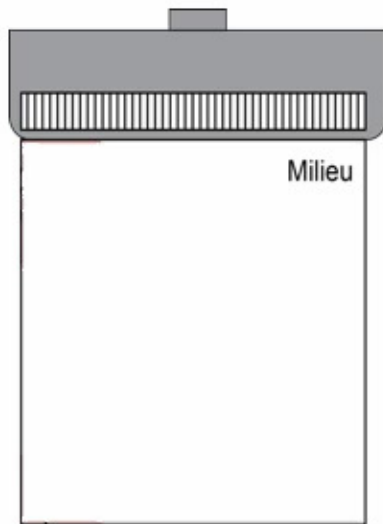


1/ Transmit focused ultrasound

1

➔ Using ultrafast imaging one can image shear wave propagation

# Ultrafast imaging of shear wave propagation

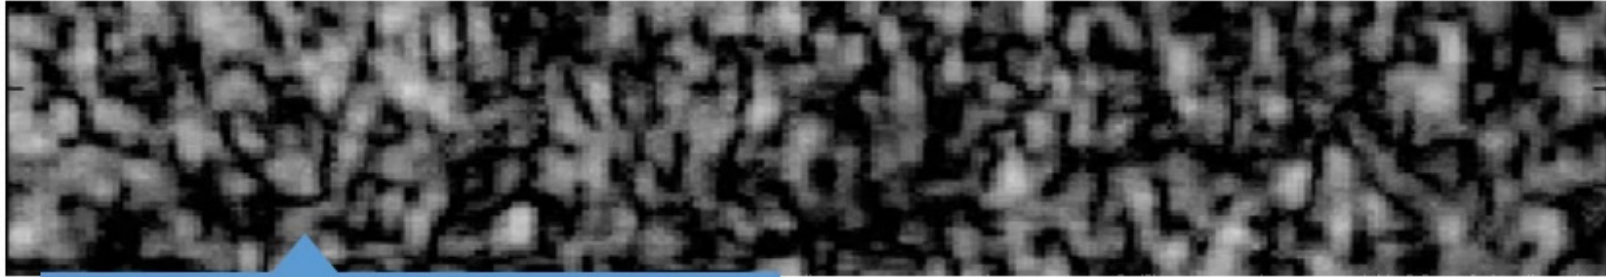


Ultrafast ultrasound movie ( 10.000 im/s)

## Local velocity estimation



# Ultrafast imaging of shear wave propagation

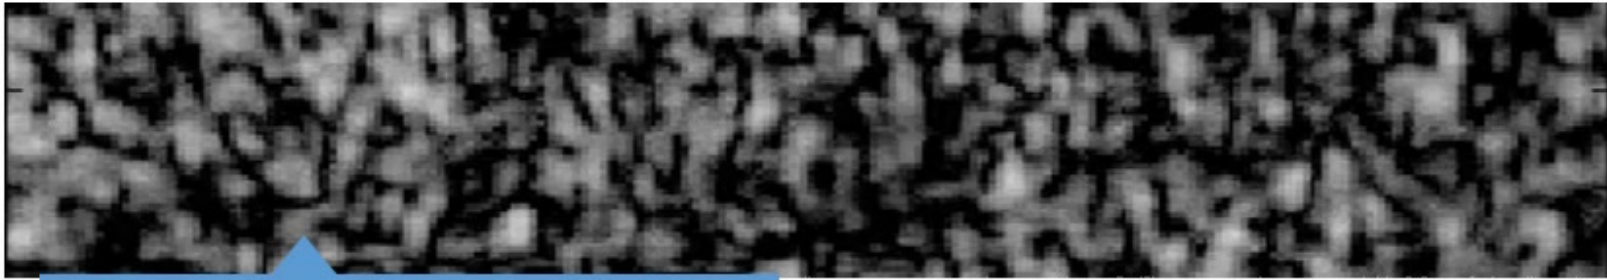

Ultrafast ultrasound movie ( 10.000 im/s)

# Shear wave elastography in the Supersonic Imagine system

The shear wave is induced using the US probe and the so-called push-beam

Ultrafast imaging is performed to image the shear wave propagation










## Supersonic shear imaging



1

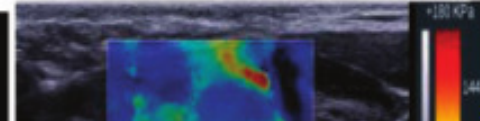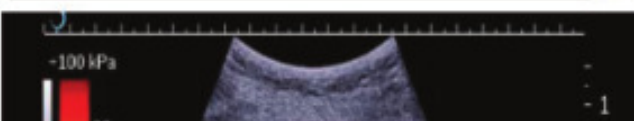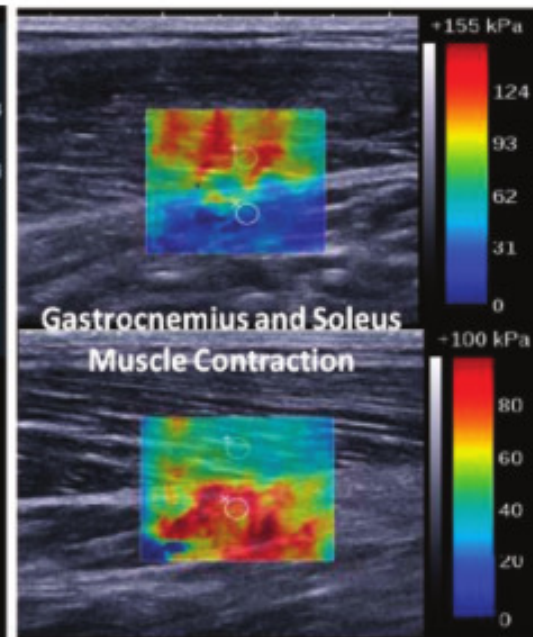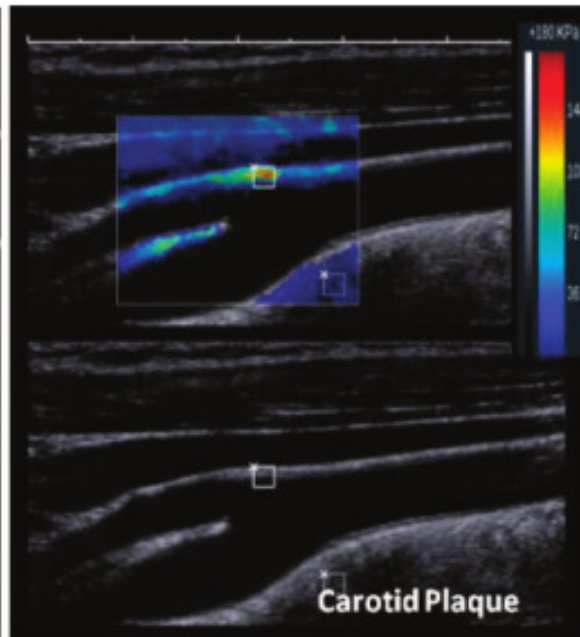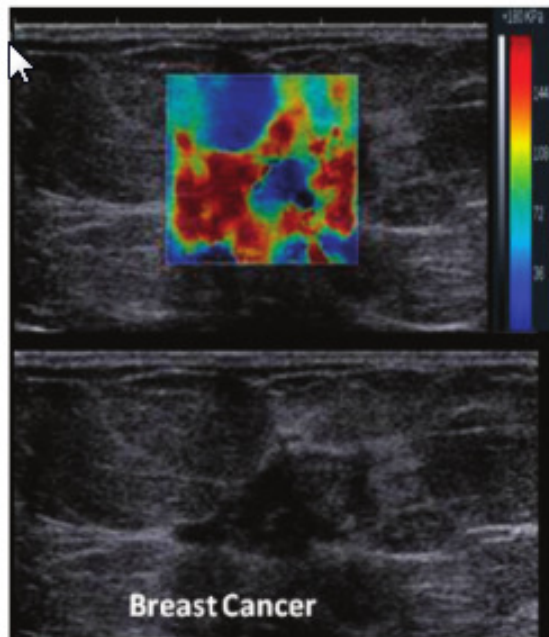


Ultrafast imaging can do many things  
2 examples:

1) Complex motion visualization:

- Blood flow
- Cardiac flow
- Arterial wall motion


2) Functional imaging of the Brain

# 1) Complex motion visualization: blood flow

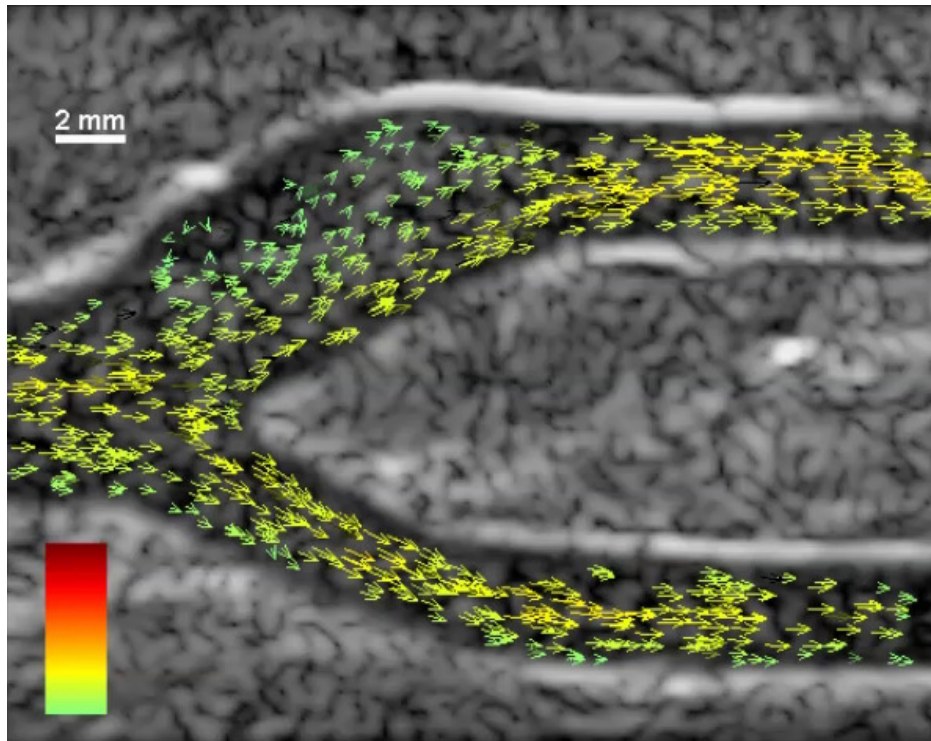

Ultrafast vector flow in  
the carotid bifurcation of  
a healthy subject

# 1) Complex motion visualization: blood flow



Ultrafast vector flow in the carotid  
bifurcation of a subject with 50%  
eccentric stenosis



# 1) Complex motion visualization: cardiac flow

- Perimembranous ventricular septal defect (significant shunt)
- 36 days old, 4259 gr.


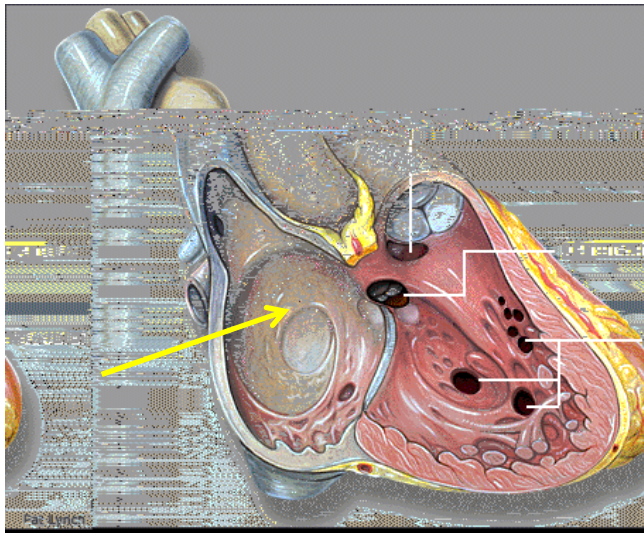


Image source: Wikipedia, Pat Lynch




Courtesy of Lasse Lovstakken, NTNU Trondheim, Norway

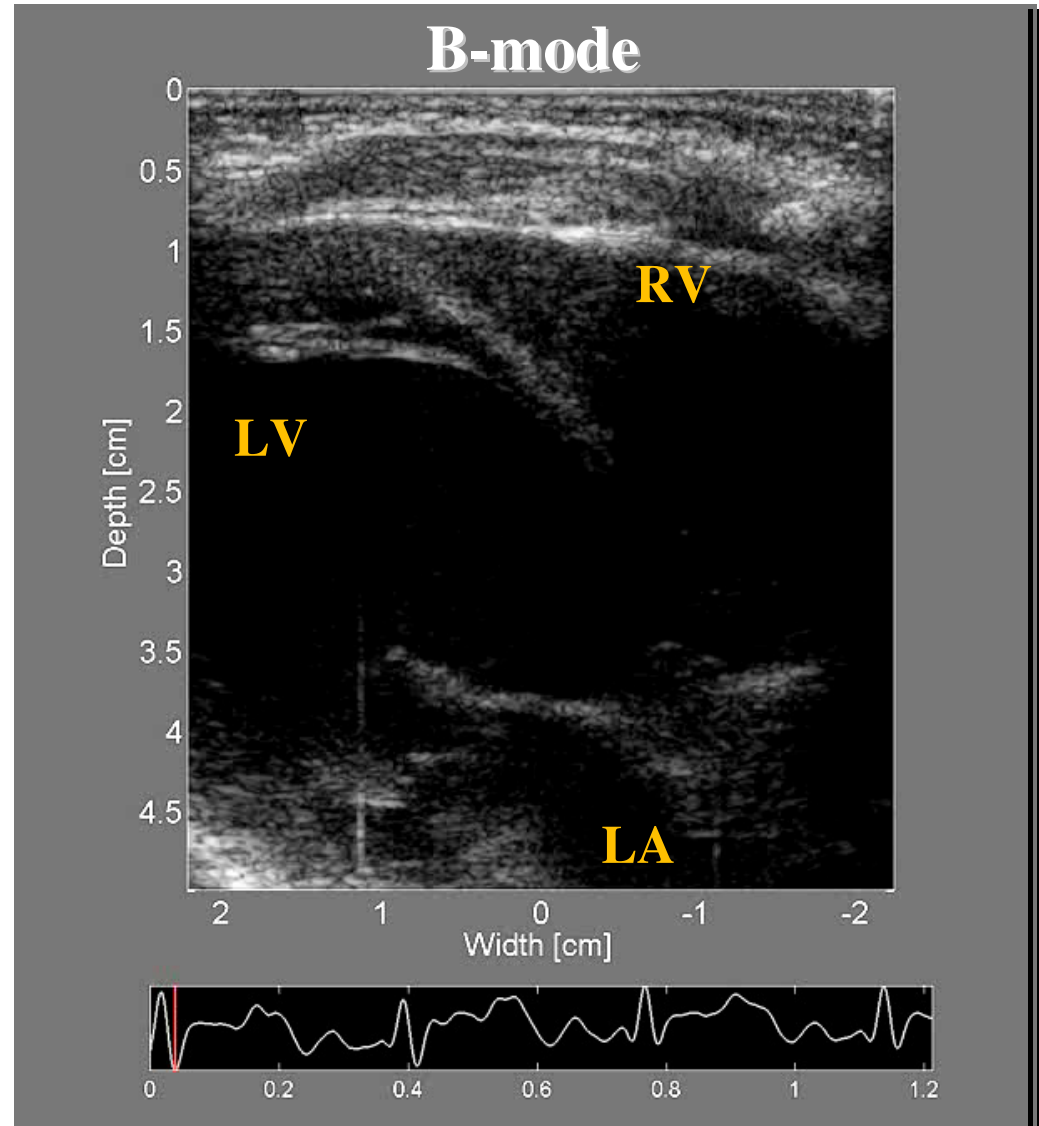


# 1) Complex motion visualization: arterial wall motion

Phantom:	Acquisition:
An PVA Cryogel artery phantom	Ultrasonix MDP
Outer / inner diameter = 9.0 mm / 7.0 mm	128 channels Sonix Daq
peak flow rate = 8.0ml/s	Linear array L14-5W/60 128 elements ; pitch = 472 $\mu\text{m}$ ; $f_0 = 5\text{MHz}$
duty cycle = 10%	PRF = 5000 Hz No compounding $\rightarrow$ 5000 images/s

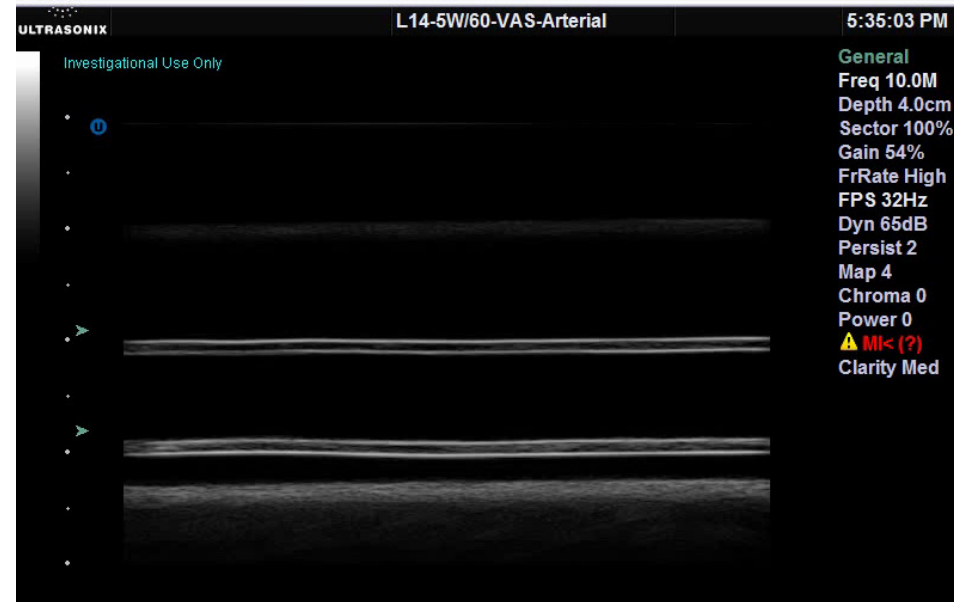


# 1) Complex motion visualization: arterial wall motion

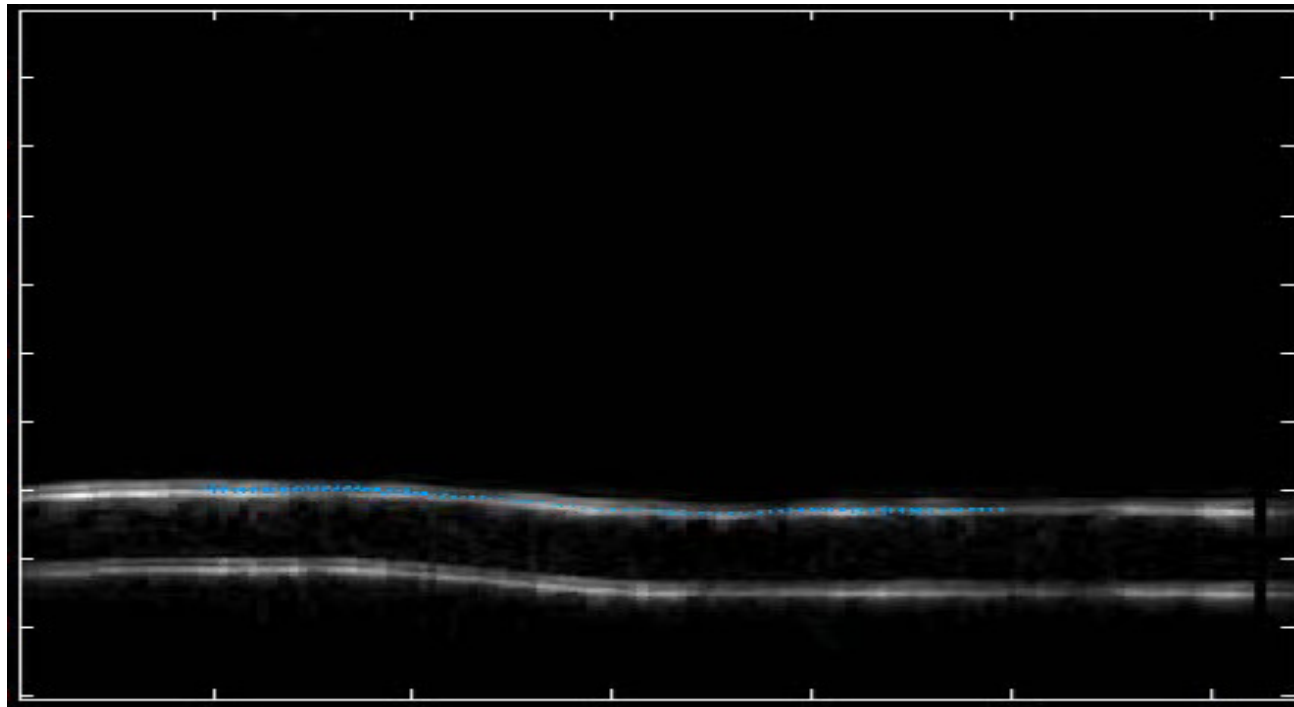

Velocity vector of the arterial wall

# 1) Complex motion visualization: arterial wall motion

*In vivo* healthy volunteer carotid artery

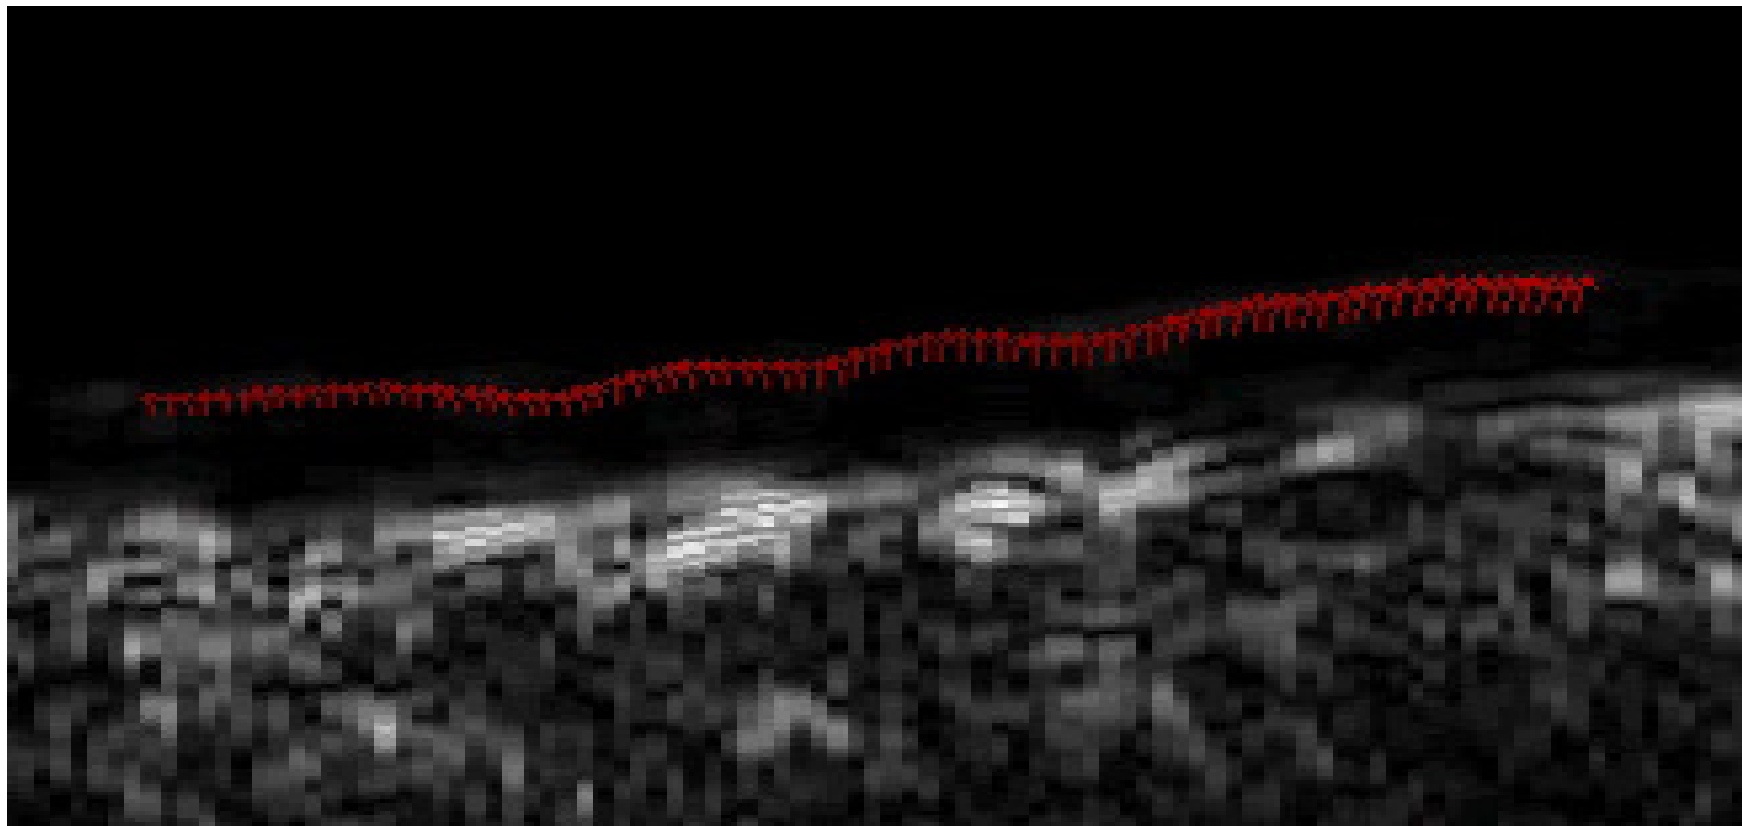

27

## 2) Functional imaging of the brain

Activation of the different parts of the brain is linked with an increase in blood flow


Power Doppler can give an indication of the quantity of flow in a region

For small quantities of blood conventional technique are not sensitive enough

Functional imaging of the brain with ultrasound is done by combining ultrafast imaging and power Doppler <sup>28</sup>


## 2) Functional imaging of the brain

In vivo proof of this concept was shown by imaging changes of cerebral blood volume in the micro vascularization of trepanned rat brain during whisker stimulation

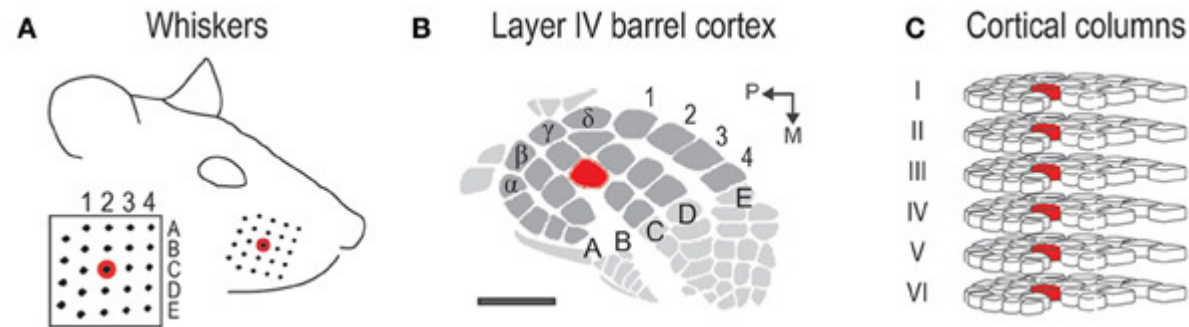

Chen Bee et. al., Front. Neural Circuits, 2012


Functional ultrasound imaging during excitation of the whiskers. Activation was clearly detected showing the excellent sensitivity and resolution of fUs imaging

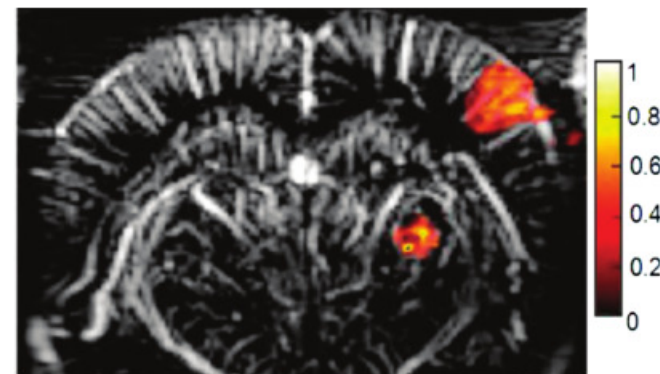

29

Mace et.al. Nature Methods, 2011

## 2) Functional imaging of the brain

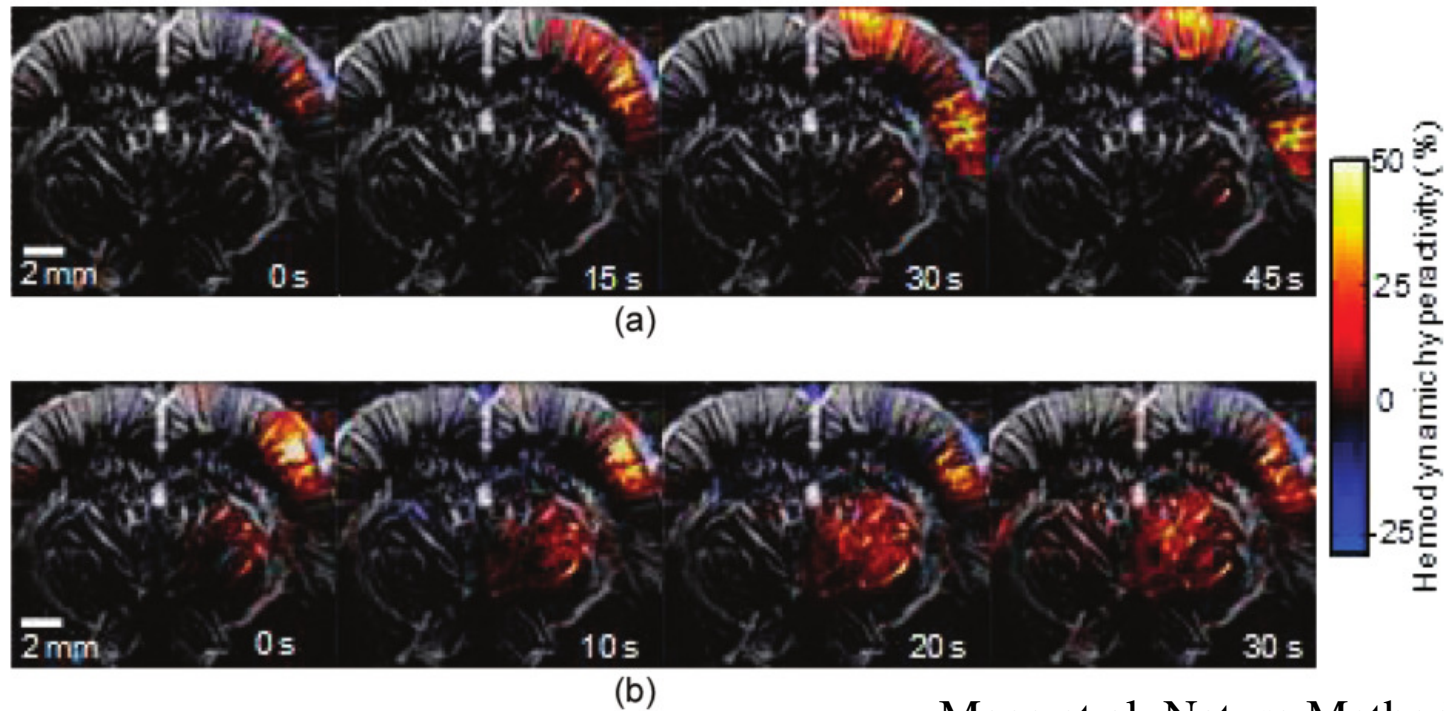

Mace et.al. Nature Methods, 2011

Spatiotemporal spreading of epileptiform activity for two ictal events. Brain cerebral blood volume (cBV) changes (% relative to the baseline) are superimposed on a control baseline cBV image. In (a) we can see an onset and a cortical propagation. In (b), the activity is seen spreading in the thalamus.

## 2) Functional imaging of the brain

Amazing potential of functional imaging of the brain by ultrasound.

One example: Imaging of the cerebral activity during fetal growth....

# Examples and the corresponding evolution of ultrasound imaging





- static elastography
- shear wave elastography
- ultrafast imaging
- photo-acoustic imaging

Part 2







# WHY Photo-acoustic imaging?






## Optical imaging

-  Contrast
-  Resolution  $> \sim 1 \text{ mm}$
-  Investigation depth  $< \sim 5 \text{ cm}$
-  Functional information


## Ultrasound imaging


-  Contrast
-  Resolution  $> \sim 100 \mu\text{m}$
-  Investigation depth  $\sim 10 \text{ cm}$
-  No Functional information

## Photo-acoustic imaging

-  Contrast (optical absorption)
-  Resolution of Ultrasound
-  Depth of investigation
-  Functional information due to optical absorption
-  Non invasive, non ionizing


# Physical principle

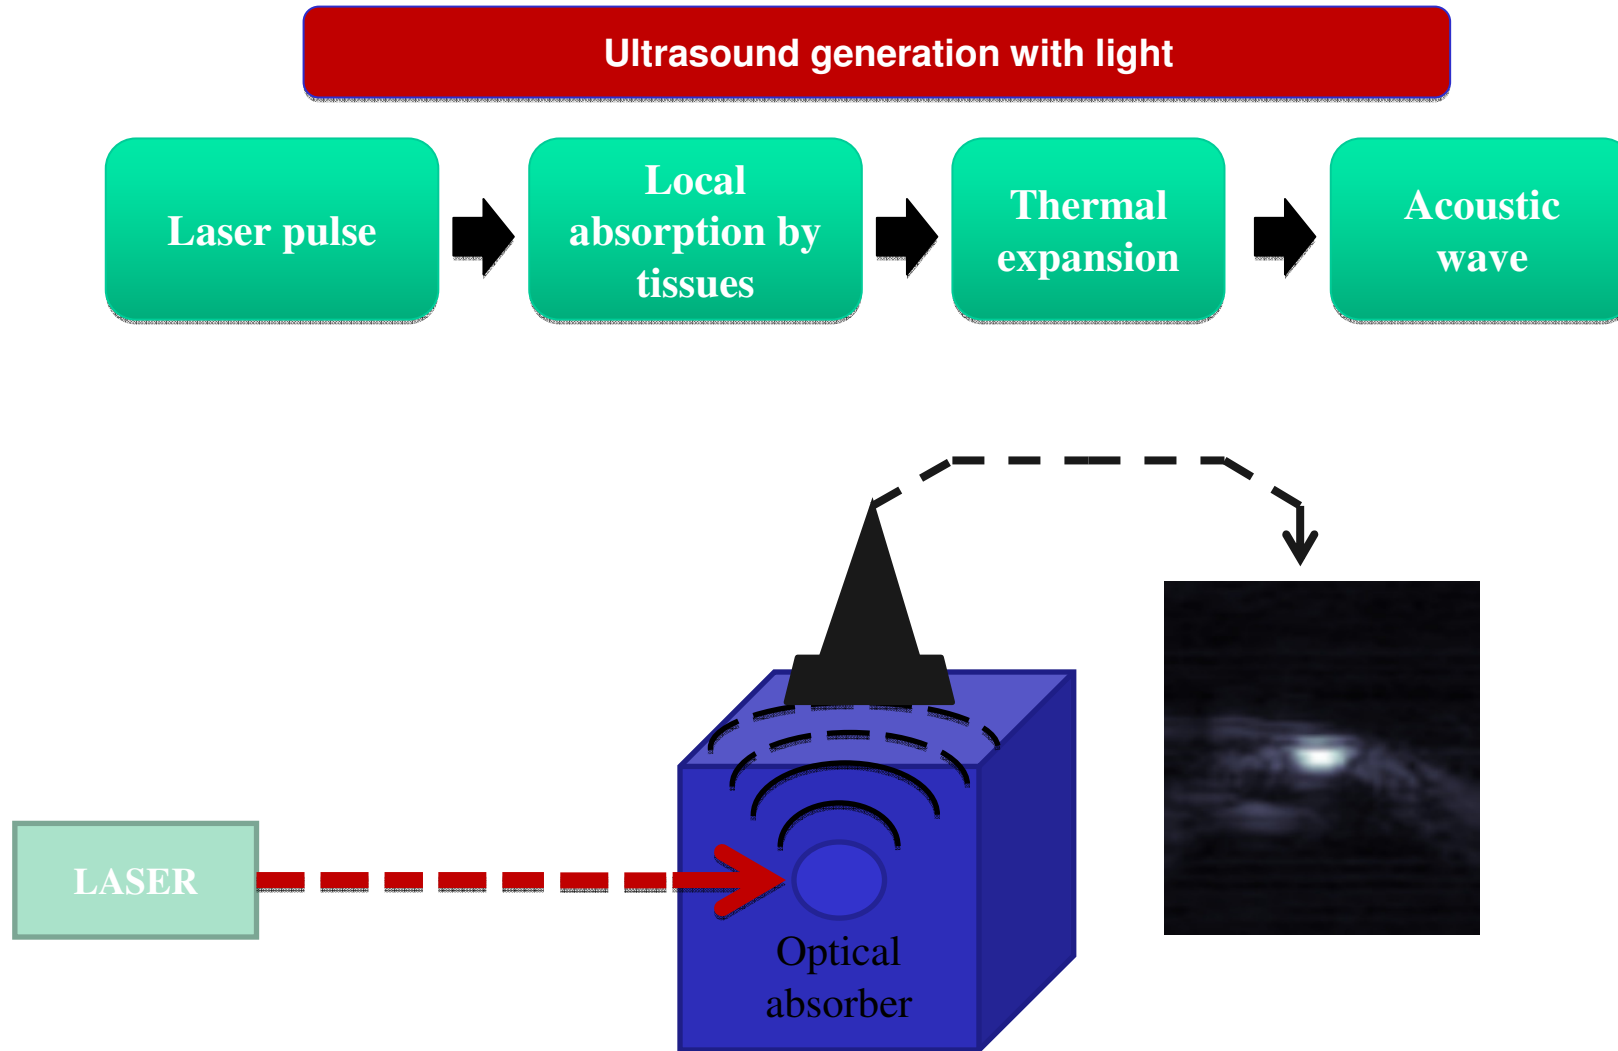

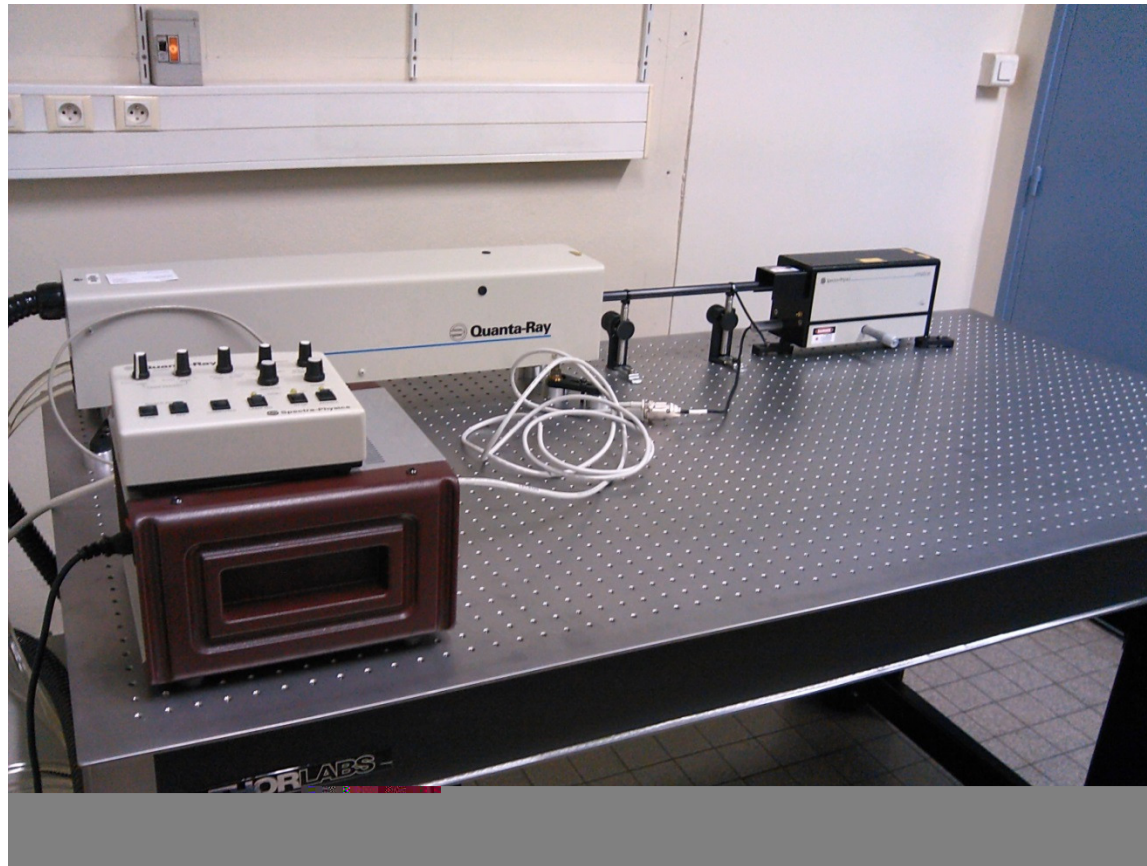

Courtesy of François Varray, CREATIS, University of Lyon



# Acquisition setup

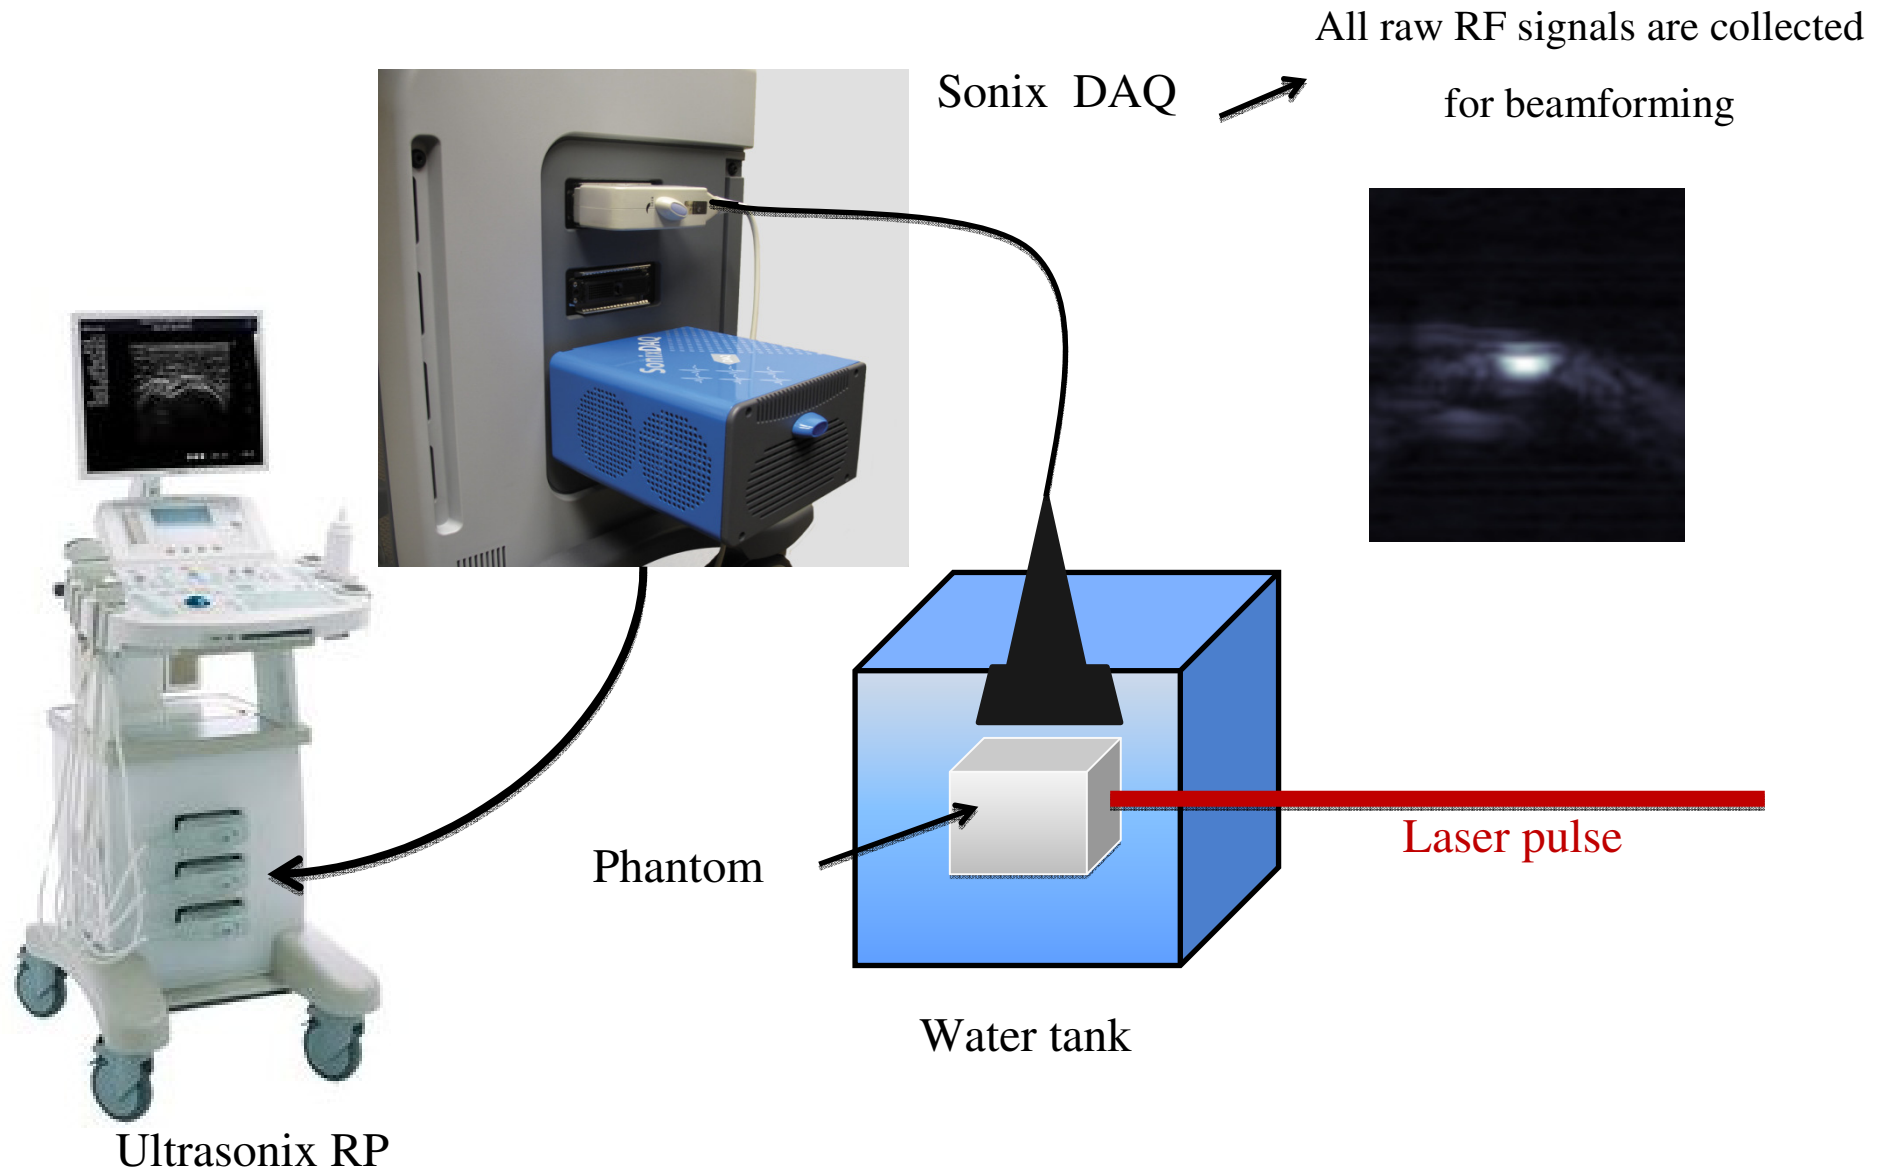

Courtesy of François Varray, CREATIS, University of Lyon

# Simple experiment with wires as absorber

- Several optical absorbers

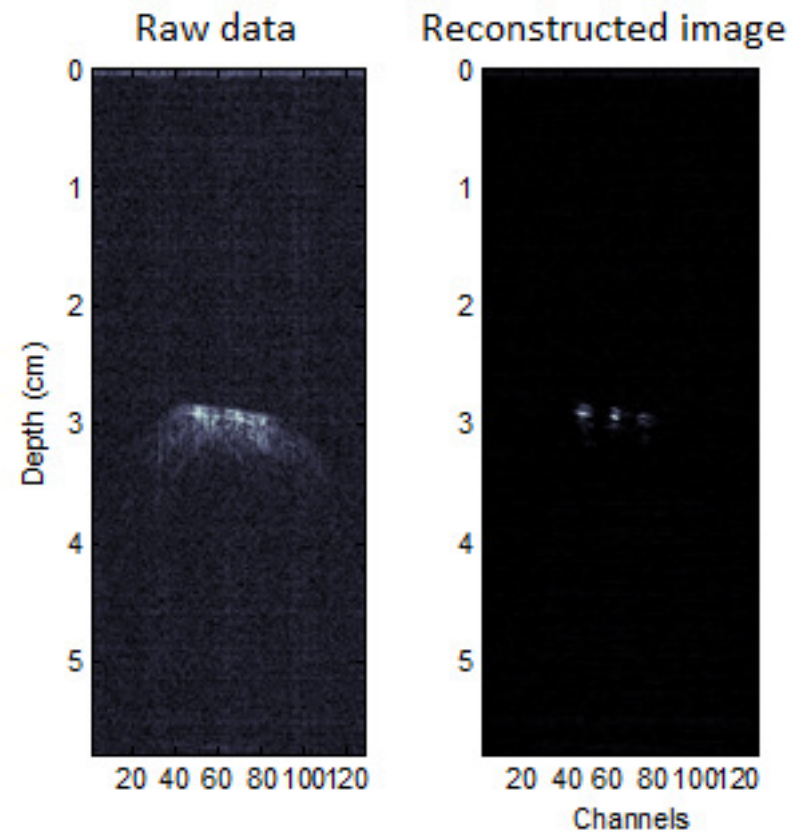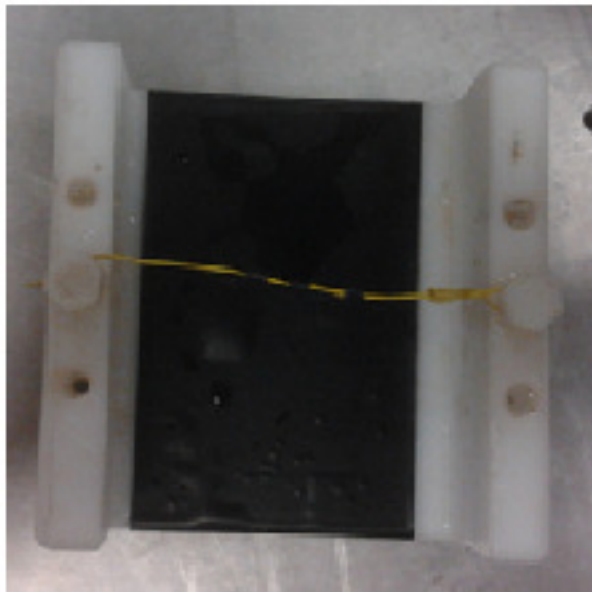


Courtesy of François Varray, CREATIS, University of Lyon


# Applications

Vascularization

Cancer → abnormal vascularization

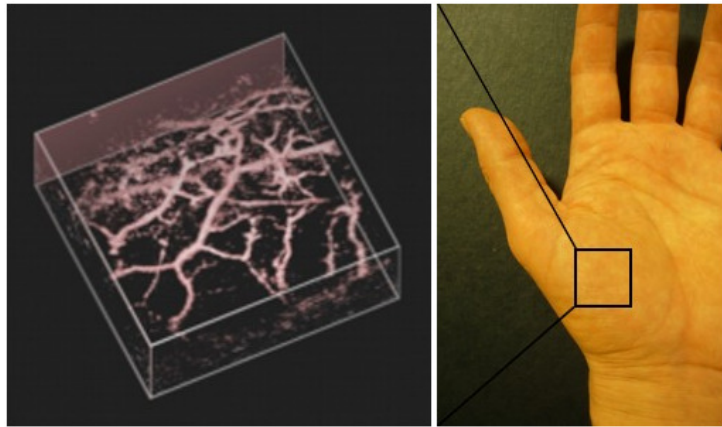


In vivo PA image of the hand vascularization. *UCL PA Imaging Group*

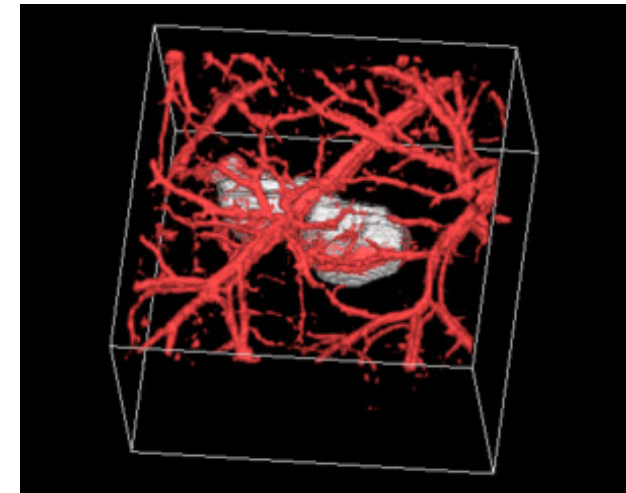


3D photoacoustic imaging of melanoma *in vivo*. *Zhang et.al. Nature Biotechnology 2006*



# Applications

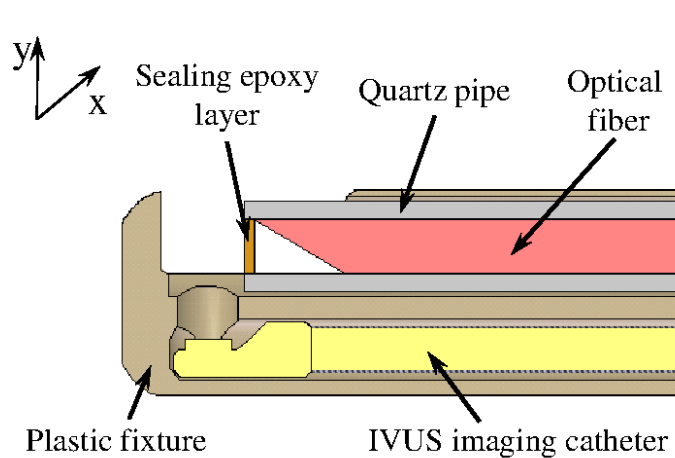


(a)

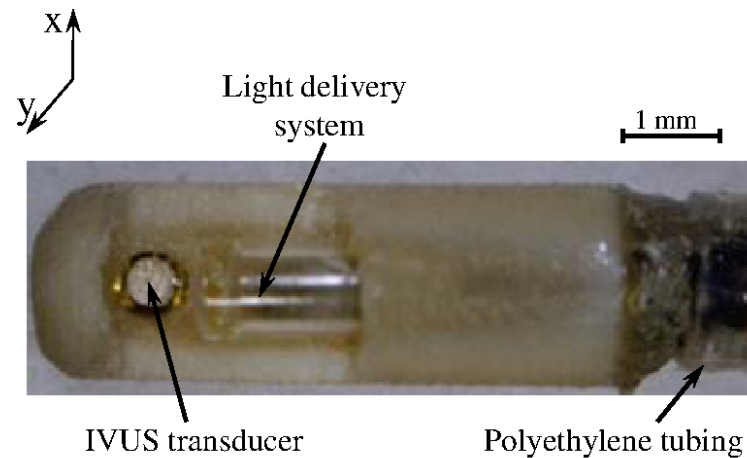

(b)


Karpiouk et.al, *J. Biomed. Opt.*  
2012

Intra-vascular photo-acoustic,  
vascularization of the plaque

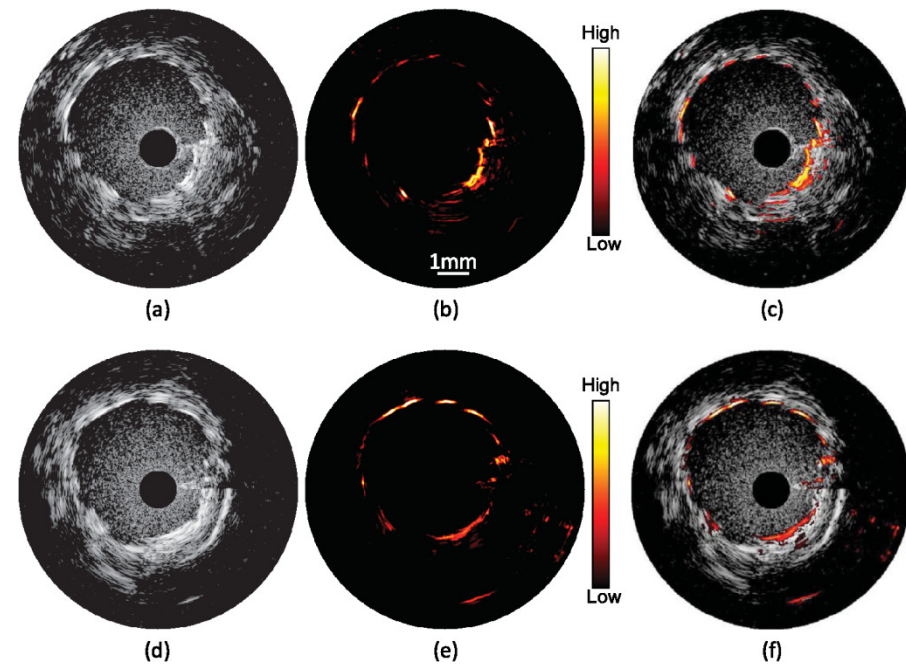

# Applications

## Functional imaging of the brain

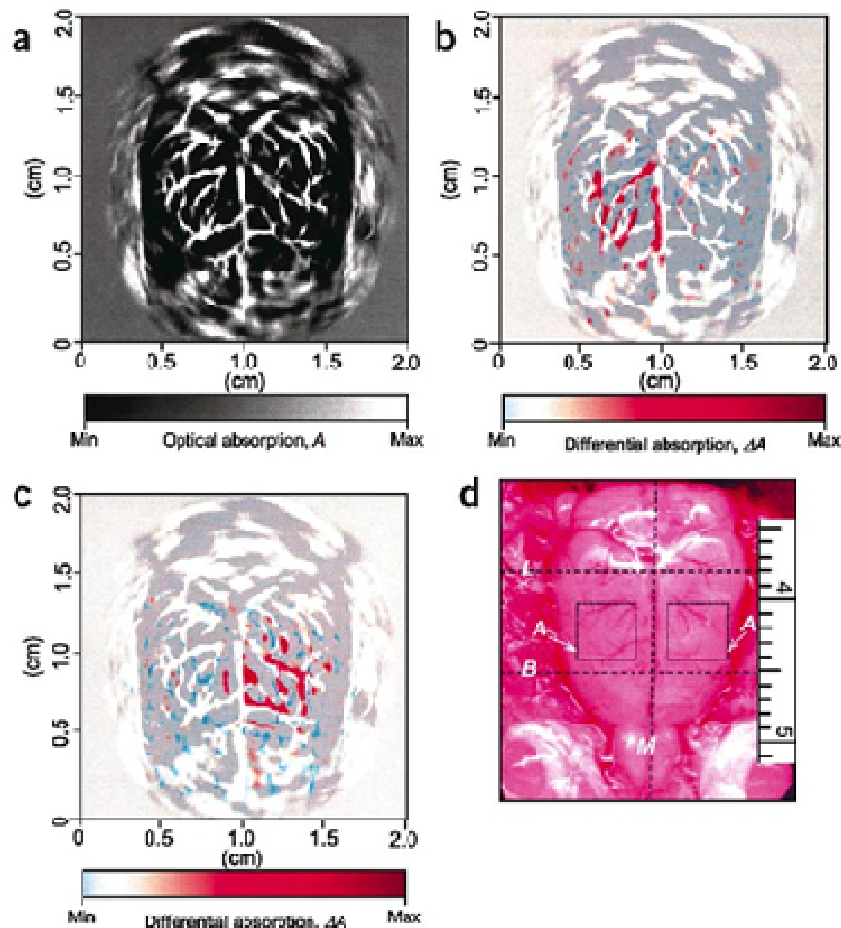

Cerebral hemodynamic changes in response to whisker stimulation, Wang et. al. *Nature Biotechnology*, 2003



# Ultrasound advanced imaging: beyond anatomy!

- Elasticity
- Cardiac function
- Vector flow
- Arterial wall motion
- Functional imaging of the brain (ultrafast imaging or photo-acoustics)
- Vascularization using photo-acoustics